

MTTS Light Meter

Model: LM-800



User Manual

Effective date: January 2021
Issue Number: 02 Version: 00 EN
Issue Date: November 2021



Contents

Company Information	04
Introduction	05
Device Description	06
Warnings	08
Operation	09
Alarm System	12
Cleaning	13
Maintenance and Service	14
Specifications	17
Explanation of Symbols	19
Warranty Policy	20



PROMETEO SRL
Via Mantova 9
38122 Trento
Italy



WARNING - a warning statement refers to the conditions when the possibility of injury to the patient or user exists if a procedure is not followed correctly.



NOTE - a note statement provides additional information intended to clarify points, procedures or instructions.



This user manual is intended for health care professionals.




The Light Meter is to be operated by qualified personnel only. This manual, all precautionary information, and specifications should be read before use.

The MTTS Light Meter is a spectroradiometer for measuring the irradiance (radiant power) of neonatal phototherapy lights and bili-beds.


Device Description

Device Description

The MTTs Light Meter is single measurement unit suitable for overhead and bed type phototherapy. It has 2 sensors loc on both sides of the meter.

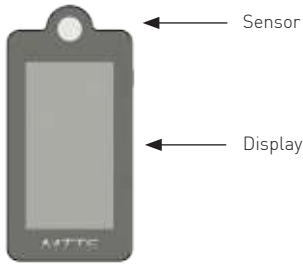

LCD screen is a 'touch type'. Place the finger on the touch panel, do not press hard

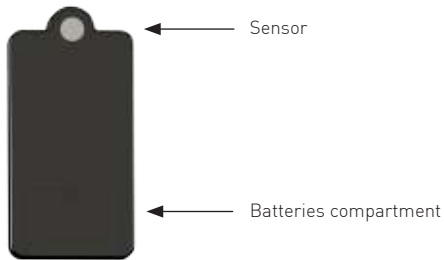

Device Description

Measuring Irradiance


The MTTs Light Meter is a spectroradiometer that measures the therapeutic irradiance (radiant power) of neonatal phototherapy lights. It measures the irradiance of the wavelengths from 400 to 500 nanometers (nm), the blue-green portion of the spectrum, which includes the principal action spectrum of bilirubin. The device accounts for cosine correction allowing more light from different angles.

Units of Measurement





The MTTs Light Meter measures irradiance in units of microwatts per square centimeter per nanometer ($\mu\text{W}/\text{cm}^2/\text{nm}$). A nanometer is a measure of wavelength equal to one-billionth of a centimeter. The term "per nanometer" indicates the average irradiance per nanometer across the spectral band being measured, which is 100 nm wide. This makes it possible to compare average irradiance across spectral bands of different widths.

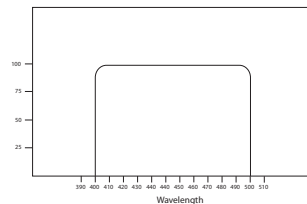
Instrument Response Characteristics

The figure below represents the nominal response characteristics of the MTTs Light Meter, which matches the action spectrum of bilirubin as closely as possible.



Warnings


-  Explosion hazard. Do not use this device in the presence of flammables (e.g., oxygen, nitrous oxide, anesthetics).
-  Read and be familiar with this instruction manual before using this device.
-  Only use this device under the direct supervision of a licensed medical practitioner.
-  Inspect this device before each use to ensure proper functioning.

 The hospital/facility is responsible for ensuring that all personnel who operate or maintain this device are trained in its operation and safe use, and for maintaining training records of attendance and evidence of understanding.


Operation

Taking Measurements - Overhead Phototherapy

1. Turn the MTTs Light Meter on.

 LCD screen is a 'touch type'. Place the finger on the touch panel, do not press hard

2. Hold the MTTs Light Meter against the infant's body as near to the umbilical as possible and aim the Light Meter at the center of the phototherapy light (see figure below).

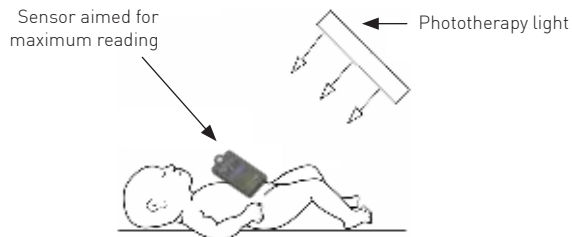

- For reproducible measurements, always hold the sensor on the same place on the infant's body.
- Changes in the distance or angle of the light to the patient will change the irradiance the patient receives, requiring new measurements to be taken.

Operation

3. Read irradiance measurement from the display. Adjust the aim of the MTTs Light Meter sensor to obtain the maximum reading.
4. The reading value is displayed for 5 seconds after the measurement
5. Touch on/off button to turn MTTs Light Meter off. MTTs Light Meter automatically shuts off after 1 minute to preserve battery life.

i If more than one phototherapy light is being used on the infant, take separate measurements for each light and chart each reading.

Operation


Taking Measurements - Bili-Bed Phototherapy

1. Turn the MTTs Light Meter on.

i LCD screen is a 'touch type'. Place the finger on the touch panel, do not press hard

2. Place the MTTs Light Meter in the middle of the lighted side of the pad or mattress (see figure below). Any disposable covers should be on the pad or mattress.

MTTs light meter

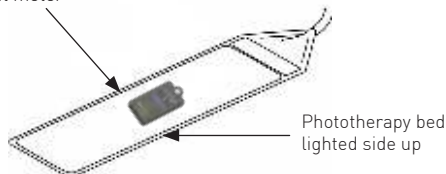

3. Read irradiance measurement from the display. Adjust the aim of the Light Meter sensor to obtain the maximum reading.
4. Take two additional readings at different places on the pad, then average all three readings.
5. Touch on/off button to turn the Light Meter off. The Light Meter automatically shuts off after 1 minute to preserve battery life.

i If a Bili-Bed is being used at the same time as an overhead phototherapy light the Light Meter displays combined value of both units.

Alarm System

1. Low battery - Battery power is low
replace the battery (see page 10)
2. System failure - contact the authorized representative
3. Out of measurement - the light irradiance is outside the
measurement range of the device

Cleaning

Required items:



Clean
Cloth






Mild
Detergent

To clean the Light Meter:

1. Confirm that the Light Meter is off. If it is on, press POWER to turn it off.
2. Dampen the cloth with either the mild soap-and-water solution or detergent, then wipe down all exterior surfaces of the Light Meter.

Maintenance and Service

-  Only qualified technicians should maintain or service this device.
-  Read and be familiar with this instruction manual before using this device.
-  The printed circuit boards (PCBs) contain static sensitive parts. Always use appropriate electrostatic discharge protection, such as an electrical-grounding wrist strap, when working with internal components.


Replacing the Batteries

Required items:

2 x AAA/LR6/1.5V alkaline, non-rechargeable batteries

To replace the battery:

1. Remove the back cover
2. Insert the new 1.5-volt batteries into the battery holder

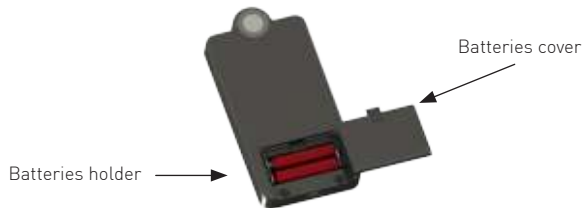

Maintenance and Service

Calibrating the Light Meter


The MTTs Light Meter was factory calibrated to a radiometric standard in accordance to the National Institute of Standards and Technology (NIST). The Calibration Certificate is enclosed with this the device.

To assure continued accurate measurement of irradiance, the MTTs Light Meter should be recalibrated every **24 months** to a radiometric (irradiance) standard. Because certain calibration factors are stored in the Light Meter memory, the Light Meter must be recalibrated at MTTs. The date of the last calibration is labeled on the Calibration Certificate.

Both the readout and sensor should be returned for calibration. The Light Meters under warranty are recalibrated at no cost. Others are recalibrated at nominal cost. For information on returning the Light Meter, see below.

Service and Repair

The MTTs Light Meter has no customer serviceable parts, and must be returned to MTTs for all repairs and parts replacement. After any service, the Light Meter must be recalibrated radiometrically to assure accurate measurement of irradiance.

-  Customer attempts to service the Light Meter will invalidate the warranty and may result in irreparable damage

Maintenance and Service

Returning for Service

When sending equipment for service:

- Contact MTTs Technical Service for a Return Merchandise Authorization (RMA) number and the location where the equipment should be sent.

- Clean the device, securely package it, and include the RMA number on the outside of the box.

- In the Asia, ship the equipment to:
Medical Technology Transfer and Services (MTTS) Ltd
No 26 Lane 41 An Duong Vuong
Tay Ho, Hanoi

Specifications

Performance Specifications

Control Settings

Spectral response		400-500 nm
Measuring range	single side	0.0 – 150.0 $\mu\text{W}/\text{cm}^2/\text{nm}$
	double side	0.0 – 300.0 $\mu\text{W}/\text{cm}^2/\text{nm}$
Resolution		0.1 $\mu\text{W}/\text{cm}^2/\text{nm}$
Cosine characteristics		$\pm 2\%$ @ 30 degree angle
		$\pm 7\%$ @ 60 degree angle
		$\pm 25\%$ @ 80 degree angle
Accuracy		+/- 3%

Displays

Characteristics	Touch LCD
Features	auto-zeroing, self-check, auto-off after 1 min, results display for 5 sec
Indicators	low battery, system failure, out of measurement

Physical Specifications

Dimensions (HxWxD)	148 x 73 x 17 mm
Total unit mass	200 g

Electrical Specifications

Battery	2 x AAA 1.5V alkaline batt, non-recharg.
Operational Duration	Up to 120h

Environmental Specifications

Operating	Ambient temperature 10°C to 40°C Humidity: 30% to 90% RH non condensing Atmospheric Pressure: 70-106kPa
Transport and storage	Ambient temperature 0°C to 50°C Humidity: 5% to 90% RH non condensing Atmospheric Pressure: 70-106kPa
Exclusions	None

Specifications

Standards for Reference

ISO 13485:2016
IEC 61010-1:2010
IEC 61326-1:2012
ROHS III

Explanation of Symbols

Explanation of Symbols



Refer to User Manual before operating this device.



Do not disassemble Light Meter unless you are an MTTTS trained technician or have been instructed to by qualified personnel.



Keep out of direct sunlight.



This device should be disposed of separately from normal household waste so that components can be recycled.



Device manufacturer.



Date of manufacture.



Serial Number



Power supply polarity



12 Volt, Direct Current, 5 Ampere



CE Marking



Name and address of European Authorized Representative

Warranty Policy

General Terms

This MTTs Limited Warranty gives you, the customer, express limited warranty rights from MTTs, the manufacturer for the duration specified on the Warranty Card. Please refer to the MTTs Website for an extensive description of your limited warranty entitlements. In addition, you may also have other legal rights under applicable law or special written agreement with MTTs. MTTs MAKES NO OTHER EXPRESS WARRANTY OR CONDITION WHETHER WRITTEN OR ORAL AND MTTs EXPRESSLY DISCLAIMS ALL WARRANTIES AND CONDITIONS NOT STATED IN THIS LIMITED WARRANTY TO THE EXTENT ALLOWED BY LOCAL LAW OF JURISDICTIONS OUTSIDE VIETNAM. MTTs DISCLAIMS ALL IMPLIED WARRANTIES OR CONDITIONS, INCLUDING ANY IMPLIED WARRANTIES OF MERCHANTABILITY AND FITNESS FOR A PARTICULAR PURPOSE. FOR ALL TRANSACTIONS OCCURRING IN VIETNAM ANY IMPLIED WARRANTY OR CONDITION OF MERCHANTABILITY, SATISFACTORY QUALITY, OR FITNESS FOR A PARTICULAR PURPOSE IS LIMITED TO THE DURATION OF THE EXPRESS WARRANTY SET FORTH ABOVE. SOME COUNTRIES DO NOT ALLOW A LIMITATION ON HOW LONG AN IMPLIED WARRANTY LASTS OR THE EXCLUSION OR LIMITATION OF INCIDENTAL OR CONSEQUENTIAL DAMAGES FOR CONSUMER PRODUCTS. IN SUCH COUNTRIES, SOME EXCLUSIONS OR LIMITATIONS OF THIS LIMITED WARRANTY MAY NOT APPLY TO YOU. FOR CONSUMER TRANSACTION, THE LIMITED WARRANTY TERMS CONTAINED IN THIS STATEMENT, EXCEPT TO THE EXTENT LAWFULLY PERMITTED, DO NOT EXCLUDE, RESTRICT, OR MODIFY BUT ARE IN ADDITION TO THE MANDATORY STATUTORY RIGHTS APPLICABLE TO THE SALE OF THIS PRODUCT TO YOU.

This Limited Warranty is applicable in all countries and may be enforced in any country or region where MTTs or its authorized service providers offer warranty service for the same product model number (subject to the terms and conditions set forth in this Limited Warranty)

Under this Limited Warranty, products purchased in one country or region may be transferred to another country or region where MTTs or its authorized service providers offer warranty service for the same product model number. Warranty terms, service availability, and service response times may vary from country or region to country or region. Standard warranty service response time is subject to change due to local parts availability. If so, your MTTs authorized service provider can provide you with details. MTTs will not alter form, fit, or function of this MTTs product to make it operate in a country for which it was never intended to function for legal or regulatory reasons. MTTs is not responsible for any tariffs or duties that may be incurred in transferring the products.

MTTs guarantees that the product that you have purchased or leased from MTTs is free from defects in materials or workmanship under normal use during Limited Warranty Period. The Limited Warranty Period starts on the date of purchase or lease from MTTs, or from the date MTTs completes installation. Your dated sales or delivery receipt, showing the date of purchase of the product, is your proof of the purchase or lease date. You may be required to provide proof or purchase or lease as a condition of receiving warranty service. You are entitled to hardware warranty service according to the terms and conditions of this document if a repair to your MTTs product is required within the Limited Warranty Period.

Unless otherwise stated, and to the extent permitted by local law, new MTTs product may be manufactured using new materials and used materials equivalent to new in performance and reliability. MTTs may repair or replace MTTs products (a) with new or previously used products or parts equivalent to new in performance and reliability, or (b) with equivalent products to an original product that has been discontinued. Replacement parts are warrantable to be free from defects in material or workmanship for ninety (90) days or, for the remainder of Limited Warranty Period of the MTTs product they are replacing or in which they are installed, whichever is longer.

Warranty Policy

MTTs will, at its sole discretion, repair or replace any components or product that manifests a defect in materials or workmanship during the Limited Warranty Period. All component parts removed under this Limited Warranty become the property of MTTs. In the unlikely event that your MTTs product has recurring failures, MTTs at its sole discretion, may elect to provide you with (a) a replacement unit selected by MTTs that is the same or equivalent to your MTTs product in performance or (b) to give you a refund of your purchase price or lease payments (less interests) instead of a replacement. This is your exclusive remedy for defective products.

Exclusions

MTTs DOES NOT WARRANT THAT THE OPERATION OF THIS PRODUCT WILL BE UNINTERRUPTED OR ERROR-FREE. MTTs IS NOT RESPONSIBLE FOR DAMAGE THAT OCCURS AS RESULT OF YOUR FAILURE TO FOLLOW THE INSTRUCTIONS INTENDED FOR THE PRODUCT.

This Limited Warranty does not apply to expendable or consumable parts and does not extend to any product from which the serial number has been removed or that has been damaged or rendered defective (a) as a result of accident, misuse, abuse, contamination, improper or inadequate maintenance or calibration (if required) or other external causes; (b) by operation outside the usage parameters stated in the user documentation shipped with the product; (c) by software, interfering parts or supplies not supplied by MTTs; (d) improper site preparation or maintenance; (e) virus infection; (f) loss or damage in transit; or (g) by modification or service by anyone other than (i) MTTs personnel, (ii) an MTTs authorized service provider, or (iii) your own installation of end-user replaceable MTTs or MTTs approved parts if available for your MTTs product in the servicing country or region.

Limitation of Liability

IF YOUR MTTs PRODUCT FAILS TO WORK AS WARRANTED ABOVE, THE MAXIMUM LIABILITY OF MTTs UNDER THIS LIMITED WARRANTY IS EXPRESSLY LIMITED TO THE LESSER OF THE PRICE YOU HAVE PAID FOR THE PRODUCT OR THE COSTS OF REPAIR OR REPLACEMENT OF ANY HARDWARE COMPONENTS THAT MALFUNCTION IN CONDITIONS OF NORMAL USE.

EXCEPT AS INDICATED ABOVE, IN NO EVENT WILL MTTs BE LIABLE FOR ANY DAMAGES CAUSED BY THE PRODUCT OR THE FAILURE OF THE PRODUCT TO PERFORM, INCLUDING ANY LOST PROFITS OR SAVINGS OR SPECIAL, INCIDENTAL, OR CONSEQUENTIAL DAMAGES. MTTs IS NOT LIABLE FOR ANY CLAIM MADE BY A THIRD PARTY OR MADE BY YOU FOR A THIRD PARTY.

THIS LIMITATION OF LIABILITY APPLIES WHETHER DAMAGES ARE SOUGHT, OR CLAIM MADE, UNDER THIS LIMITED WARRANTY OR AS A TORT CLAIM (INCLUDING NEGLIGENCE AND STRICT PRODUCT LIABILITY), A CONTRACT CLAIM, OR ANY OTHER CLAIM. THIS LIMITATION LIABILITY CANNOT BE WAIVED OR AMENDED BY ANY PERSON. THIS LIMITATION OF LIABILITY WILL BE EFFECTIVE EVEN IF YOU HAVE ADVISED MTTs OF THE POSSIBILITY OF ANY SUCH DAMAGES. THIS LIMITATION OF LIABILITY, HOWEVER, WILL NOT APPLY TO CLAIMS FOR PERSONAL INJURY.

THIS LIMITED WARRANTY GIVES YOU SPECIFIC LEGAL RIGHTS. YOU MAY ALSO HAVE OTHER RIGHTS THAT MAY VARY FROM COUNTRY TO COUNTRY. YOU ARE ADVISED TO CONSULT APPLICABLE COUNTRY LAWS FOR A FULL DETERMINATION OF YOUR RIGHTS.

Warranty Policy

Limited Warranty Period

The Limited Warranty Period for this MTTS product is a specified, fixed period commencing of the date of purchase and specified on the Warranty Card. The date on your sales receipt is the date of purchase unless MTTS or your reseller informs you otherwise in writing.

Customer Responsibilities

In order to avoid the risk of charges for issues not covered by your limited warranty (issues that are not due to defects in materials and workmanship on MTTS product), you will be asked to assist MTTS as follows:

- Verify configurations, load most recent firmware, install software patches, run MTTS diagnostics and utilities;
- Implement temporary procedures or workarounds provided by MTTS while MTTS works on permanent solution;
- Cooperate with MTTS in attempting to resolve the problem using online chat, email, or telephone. This may involve performing routine diagnostic procedures, installing additional software updates or patches;
- Perform additional tasks as defined within each type of warranty service provided by MTTS and any other actions that MTTS may reasonably request in order to best perform the warranty support

CUSTOMER IS RESPONSIBLE FOR DELIVERING THE PRODUCT (AND ALL COSTS INVOLVED) FROM HIS LOCATION TO THE MTTS AUTHORIZED SERVICE POINT.

Contacting MTTS

If your MTTS product fails during the Limited Warranty Period and the suggestions in the product documentation do not solve the problem, you can receive support by doing one of the following:

- Locate and contact your nearest MTTS service provider via MTTS website:
<http://www.mtts-asia.com/support/>
- Call the Technical Support Centre:
+84 24 3766 6521

Before calling MTTS or an MTTS authorized service provider please have the following information available:

- Product serial number and model name
- Applicable error messages
- Detailed questions



EC REP

PROMETEO SRL
Via Mantova 9
38122 Trento
Italy